

pH Sensor Target: Select the SE 555 Unless...



Water & Wastewater

Low Conductivity Liquids

ETA Process Instrumentation


www.etapii.com
sales@etapii.com
tel 978.532.1330

New England

Martech Controls

www.martechcontrols.com
sales@martechcontrols.com
tel: 315.876.9120



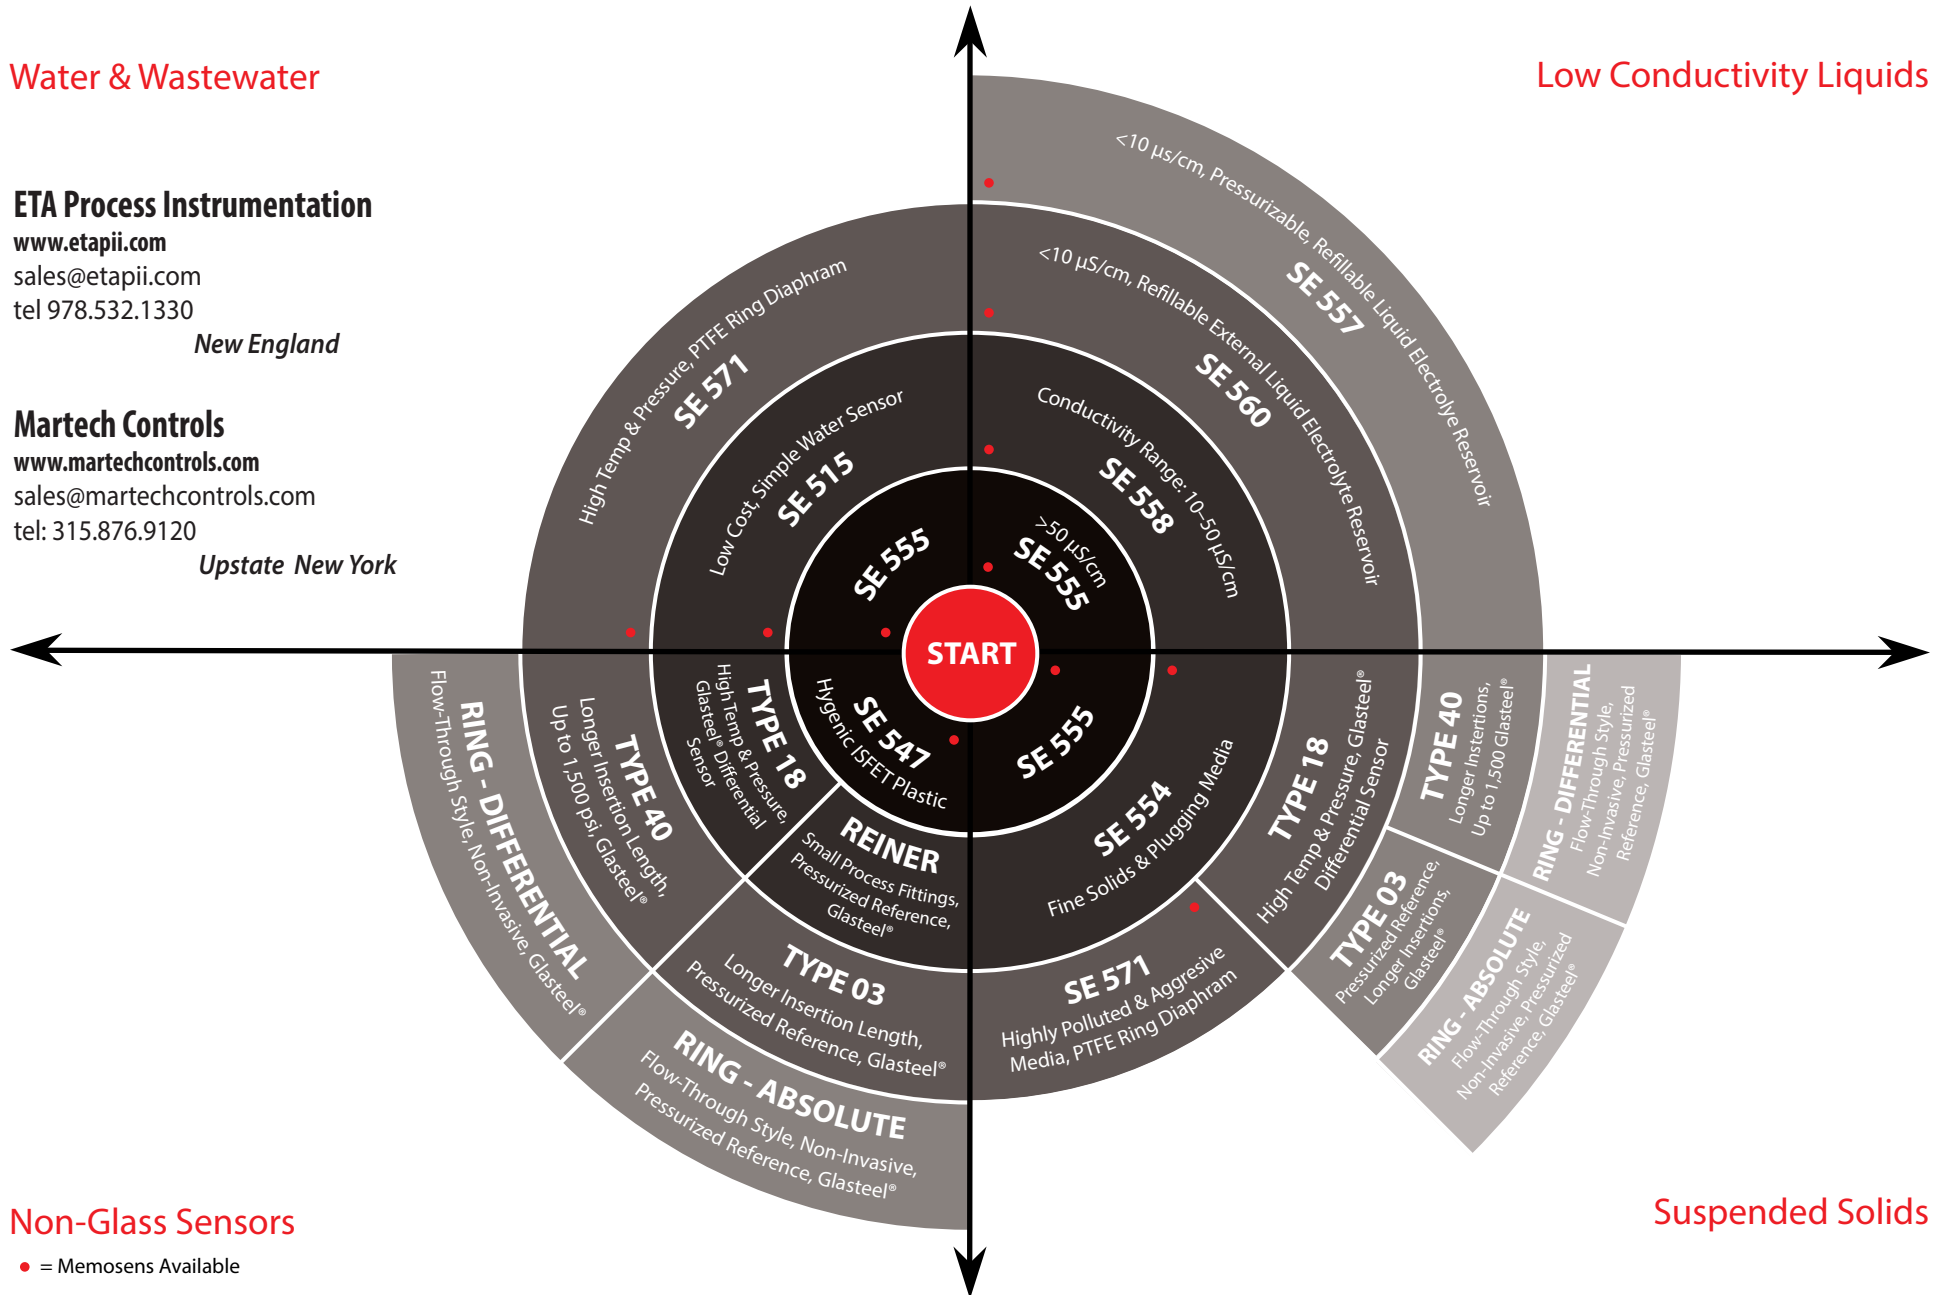












Upstate New York



• = Memosens Available

pH Sensor Selection Chart



															
	SE 515	SE 547	SE 554	SE 555	SE 557	SE 558	SE 560	SE 571	TYPE 18	TYPE 40	REINER	TYPE 03	RING	PL H-93	PL PETR
Memosens Compatible	■	■	■	■	■	■	■	■						■	
ORP			SE 564	SE 565					■	■	■	■	■		
pH & ORP			SE 554 AMSN	SE 555 AMSN											■
pH Range 0...14	■	■	■	■	■	■	■	■			■	■	■	■	■
pH Range 3...10									■	■					
CIP/SIP/ Autoclavable		■		■	■		■		■		■				
High Purity/Low Ionic Activity					■	■	■								
Glasteel - Run Dry									■	■	■	■	■		
Requires Elec- trolyte Vessel							■				■	■	■		
No Protrusion into Process Piping													■		
Junction/ Diaphragm	Ground glass sleeve	Ceramic x1 with ISFET Sensing	Open	Ceramic	Ceramic	Ceramic x3	Platinum x3	PTFE ring			Annular	Annular	Annular	PTFE ring	Open
Temperature (F°)	23...176	5...275	32...266	32...284	-4...212 0...275	23...212	-4...176	32...266	32...284	32...284 32...400	32...284	32...284	32...384	32...275	32...266
Pressure (psi)	0...58	-0.2...10	0...145	-14...174	-14...87	-14...43	-14...7	-14...174	-14...215	0...1,500	-14...87	-14...130	14... 1,218	14...180	0...180

Please refer to our product catalog excerpts for complete sensor details